

Document made available under the Patent Cooperation Treaty (PCT)

International application number: PCT/GB05/001920

International filing date: 19 May 2005 (19.05.2005)

Document type: Certified copy of priority document

Document details: Country/Office: GB
Number: 0413436.7
Filing date: 16 June 2004 (16.06.2004)

Date of receipt at the International Bureau: 23 June 2005 (23.06.2005)

Remark: Priority document submitted or transmitted to the International Bureau in compliance with Rule 17.1(a) or (b)



World Intellectual Property Organization (WIPO) - Geneva, Switzerland
Organisation Mondiale de la Propriété Intellectuelle (OMPI) - Genève, Suisse



INVESTOR IN PEOPLE

PCT/662005/001920


The Patent Office
Concept House
Cardiff Road
Newport
South Wales
NP10 8QQ

I, the undersigned, being an officer duly authorised in accordance with Section 74(1) and (4) of the Deregulation & Contracting Out Act 1994, to sign and issue certificates on behalf of the Comptroller-General, hereby certify that annexed hereto is a true copy of the documents as originally filed in connection with the patent application identified therein.

In accordance with the Patents (Companies Re-registration) Rules 1982, if a company named in this certificate and any accompanying documents has re-registered under the Companies Act 1980 with the same name as that with which it was registered immediately before re-registration save for the substitution as, or inclusion as, the last part of the name of the words "public limited company" or their equivalents in Welsh, references to the name of the company in this certificate and any accompanying documents shall be treated as references to the name with which it is so re-registered.

In accordance with the rules, the words "public limited company" may be replaced by p.l.c., plc, P.L.C. or PLC.

Re-registration under the Companies Act does not constitute a new legal entity but merely subjects the company to certain additional company law rules.

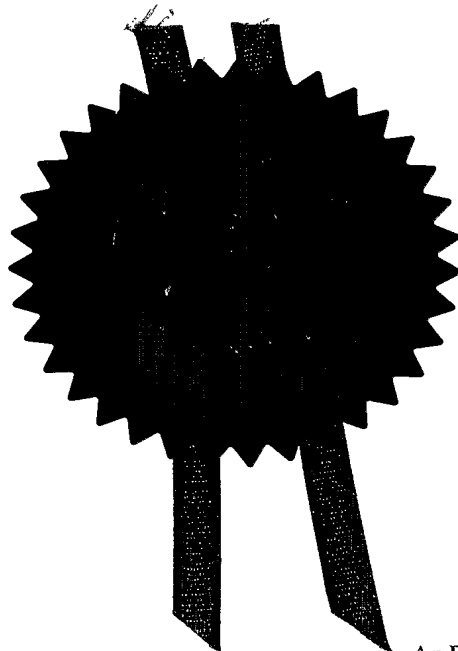


Signed *Andrew Gersey*
Dated 14 June 2005



Patents Form 1/77

The Patent Office
Cardiff Road
Newport
NP9 1RH

Request for grant of a patent

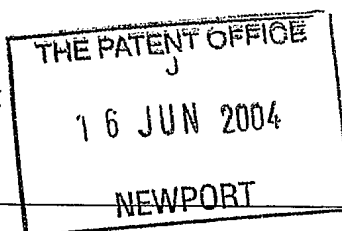

1. Your Reference

BA/RAH/Y3479

16JUN04 E904003-1 002346
P01/7700 0-20-0417436.7 NONE

2. Application number

0413436.7

16 JUN 2004

3. Full name, address and postcode
of the or each Applicant

Country/state of incorporation
(if applicable)

Nutren Technology Limited
Ribble Court
Shuttleworth Mead Business Park
Padiham
Lancashire
BB12 7SN

8879173001

Incorporated in: England

4. Title of the invention

IMPROVEMENTS IN AND RELATING TO
METABOLIC RATE MEASUREMENT

5. Name of agent

APPLEYARD LEES

Address for service in the UK to
which all correspondence should
be sent

15 CLARE ROAD
HALIFAX
HX1 2HY

Patents ADP number

190001 ✓

6. Priority claimed to:

Country

Application number

Date of filing

7. Divisional status claimed from:

Number of parent application

Date of filing

8. Is a statement of inventorship and
of right to grant a patent required in
support of this application?

YES

9. Enter the number of sheets for any of the following items you are filing with this form. Do not count copies of the same document

Continuation sheets of this form	-
Description	14
Claim(s)	-
Abstract	-
Drawing(s)	3



x 3

10. If you are also filing any of the following, state how many against each item


Priority documents	-
Translation of priority documents	-
Statement of inventorship and right to grant a patent (PF 7/77)	-
Request for a preliminary examination and search (PF 9/77)	-
Request for substantive examination (PF 10/77)	-
Any other documents (please specify)	-

11.

We request the grant of a patent on the basis of this application.
Signature Date

APPLEYARD LEES

15 June 2004



12. Contact

Ben Appleton- 0121 236 5600

IMPROVEMENTS IN AND RELATING TO METABOLIC RATE MEASUREMENT

Field of the invention

- 5 This invention relates to metabolic rate measurement apparatus and methods of measuring metabolic rate.

Background to the invention

- 10 Techniques of calorimetry are used to study energy and metabolism in humans and animals. Calorimetry is used, for example, for diagnosis of metabolic disorders and for calculating resting metabolic rate and nutritional requirements of a subject. Calorimetric measurements can
15 be made directly as a measure of heat loss of a subject, or alternatively indirect measurements can be made of a chemical by-product of metabolism. Metabolic rate can be used to determine energy expended by a subject, for example, in Kcal/minute.

- 20 Many devices are arranged to measure the resting metabolic rate of a subject, in order to determine calories expended at a resting state, which may help in diagnosis of metabolic disorders, or to monitor fitness of the subject.

- 25 In known apparatus for monitoring resting metabolic rate, the apparatus usually contains a reference data which is determined for each subject, and contains data on the average resting metabolic rate of that subject. Reference
30 data is generally inputted over a number of readings by each subject and stored as an average. When the same subject uses the device subsequently, the apparatus checks that the data inputted by the subsequent use of the

subject is within the parameters of the reference resting metabolic rate stored in the apparatus. The apparatus can immediately spot a discrepancy and report the deviation. The deviation may be due to a metabolic disorder or
5 illness in the individual, in which case the deviation may be reported to a physician or other health-care professional.

In some instances, it may be desirable for a user to be
10 able to utilise resting metabolic rate apparatus to measure metabolic other than at rest. In the known apparatus, this is not possible due to the referencing of a base metabolic rate, and the indication of an error if a subsequent use of the apparatus by the same subject is
15 outside of the reference parameters.

It would be advantageous to provide a metabolic rate measurement apparatus in which a reference data for resting metabolic rate could be inputted by each user of
20 the apparatus, but in which raised or lowered metabolic rate could be measured as and when required.

It would furthermore be advantageous to provide a metabolic rate measurement rate apparatus in which raised
25 or lowered metabolic rate could be determined by infrequent measurements, enabling a subject to input data when he or she desires, but still benefit from the apparatus calculating the raised or lowered metabolic rate.

30

It is therefore an aim of preferred embodiments of the invention to overcome or mitigate at least one of the

problems of the prior art, whether expressly disclosed herein or not.

Summary of the invention

5

According to a first aspect of the present invention there is provided a metabolic rate measuring apparatus comprising means to measure a reference metabolic rate of a user from at least one breath of the user, means to
10 measure metabolic rate from a subsequent breath of a user, means to indicate a deviation from the reference rate in a breath and prevent measuring of subsequent breaths, and means for a user to override the measurement prevention means to enable measurement of metabolic rate from breaths
15 which deviate from the reference rate.

The means to measure a reference metabolic rate may comprise an oxygen sensor and/or a carbon dioxide sensor, operatively connected to an electronic calculation means.

20

The oxygen sensor and/or carbon dioxide sensor may further be connected to a flow meter to measure the volume of inhaled and/or exhaled breaths.

25 The means to measure a reference metabolic rate may be connected to a data storage means, arranged in use to store the reference metabolic rate data.

The flow meter may comprise any suitable moveable member
30 such as a plunger or paddle wheel.

Suitable oxygen sensors include MOX-1 (RTM) sensors available from City Technology Limited, Portsmouth, UK.

The oxygen sensor and/or carbon dioxide sensor and the flow meter may be arranged to operatively co-operate to measure the reference metabolic rate.

5

The means to measure the reference metabolic rate may be the same as the means to measure metabolic rate from a subsequent breath of a user. Thus the means to measure metabolic rate from a subsequent breath of a user may
10 comprise an oxygen sensor and/or carbon dioxide sensor, and, optionally, a flow meter, connected to an electronic calculation means.

Suitably the oxygen sensor, carbon dioxide sensor and flow
15 meter, when present, transmit data to the electronic calculation means by means of electronic signals.

Preferably the means to measure the reference metabolic rate comprises means to measure a reference range of
20 metabolic rates. Thus the reference metabolic rate preferably comprises a range of values, preferably in Kcal/min.

2

The reference metabolic rate is preferably measured as an
25 average from a plurality of breaths, but may be measured from a single breath of a user.

The means to indicate a deviation from the reference metabolic rate may comprise any suitable visual or aural
30 indicator, operatively connected to the means to measure the reference metabolic rate.

Suitable visual indicators include display screens, LED indicators and the like, and the visual indicator may be in the form of text, numerals, warning lights or any mixture thereof.

5

The means to prevent measurement of subsequent breaths when a deviation from the reference metabolic rate is detected may comprise means to prevent operation of the means to measure subsequent breaths. The measurement prevention means may effect non-recordal of subsequent breaths, until a breath is measured which corresponds to the reference metabolic rate.

The means to prevent measurement of subsequent breaths may effect deactivation of the means to measure subsequent breaths. Where the means to record subsequent breaths comprise an oxygen sensor and/or a carbon dioxide sensor, they may be deactivated by the measurement prevention means.

20

The means to override the measurement prevention means may comprise means to enable operation of the means to record subsequent breaths.

The means to override the measurement prevention means may comprise an actuator, operable by a user which deactivates the measurement prevention means. The actuator may be connected to a button, lever, touch pad or the like for example, or may be user voice-activated.

30

The means to override the measurement prevention means thus enables a user to actively enable metabolic rate measurement which deviates from the parameters of the

reference metabolic rate, allowing, for example, measurement of metabolic rate during exercise, or to calculate metabolic rate after a defined time period of activity.

5

The metabolic rate measurement apparatus preferably comprises a housing having a fluid inlet. The housing preferably comprises a fluid outlet. The fluid inlet preferably comprises a mouthpiece, which may be integral with the fluid inlet, or detachable. The mouthpiece may comprise a mask, arranged in use to be secured to a user's mouth.

The metabolic rate measurement apparatus preferably comprises a portable apparatus, more preferably a handheld apparatus.

The metabolic rate measurement apparatus may be powered by an internal power source such as a power cell or battery, or may comprise means to connect the apparatus to an external power source, such as a mains electricity plug for example.

Brief description of the drawings

25

The invention will now be described by way of example only, with reference to the following drawings, in which:

Figure 1 is a schematic, partially cross-sectional, side view of part of a metabolic rate measuring apparatus in accordance with the present invention, in a start position;

30

Figure 2 is a schematic, partially cross-sectional, side view of the apparatus of Figure 1 in an end position;

Figure 3 is a schematic, partially cross-sectional, side view of a second embodiment of a metabolic rate measurement apparatus in accordance with the present invention.

Description of the preferred embodiments

10

Figures 1 and 2 show part of a metabolic rate measurement apparatus of the invention in the form of a calorimeter, suitable for calculating the metabolic rate of a subject. The apparatus 2 comprises a housing 4, means to measure the volume of a user's inhaled breath in the form of a plunger 6 and a movement sensor provided by a first switch 10 and a second switch 12. The apparatus comprises a means to measure the gas content of an exhaled breath in the form of an oxygen sensor 8. The apparatus 2 further comprises electronic calculation means 14. The plunger is slideably moveable inside the housing 4, the interior of the housing 4 and the plunger 6 having the same cross-sectional shape. The relative dimensions of the periphery of the plunger 6 and the interior of the housing 4 being arranged such that there is a substantially fluid-tight fit between the periphery of the plunger 6 and the interior of the housing 4.

The apparatus 2 also includes a means to override the measurement prevention means in the form of an actuator button 50, operably connected to the electronic calculation means 14 by a wire (not shown).

The oxygen sensor 8, the plunger 6 and movement sensor switches 10 and 12, and the electronic calculation means 14 are operably co-operable provide a means to measure a reference metabolic rate from a breath of a user, and
5 metabolic rate from subsequent breaths of a user, based on oxygen content of exhaled breath, in conjunction with the means to measure the volume of breath.

The housing 4 further comprises of a fluid inlet 16 and a
10 fluid outlet 18.

The oxygen sensor 8 is embedded in the end 20 of the plunger 6. The oxygen sensor is electrically connected to the electrical calculation means 14 by wires 22.

15

The first switch 10 of the movement sensor is embedded in a side of the plunger 4. The second switch 12 of the movement sensor is embedded in the interior wall of the housing 4. A wire 24 connects the first switch 10 with
20 the electrical calculation means 14 and a wire 26 connects the second switch 12 with the electrical calculation means 14.

In use of the apparatus 2, the plunger 6 is arranged in
25 the housing 4 at the start position as shown in Figure 1. An exhaled breath is guided into the fluid inlet 16 of the housing 4. The end of the housing 4 providing the fluid inlet 16 may act as a mouthpiece for the apparatus 2. Alternatively, a separate mouthpiece (not shown) may be
30 directly or indirectly connected to the housing 4. The exhaled breath causes the plunger 6 to move away from the fluid inlet 16. The plunger 6 will continue to move in this direction until the end 20 of the plunger 6 passes

the fluid outlet 18 to reach the end position as shown in Figure 2. Thereafter, excess exhaled breath will pass out of the fluid outlet 18 and movement of the plunger 6 will cease.

5

Whilst the plunger 6 is moving from the start position to the end position, the oxygen sensor 8 measures fraction of oxygen in the exhaled breath. The oxygen sensor 8 sends information of the measurement to the electrical calculation means 14 in the form of an electrical signal by means of wire 22. The electrical calculation means calculates the reference metabolic rate of a user based on data received from the movement sensor and oxygen sensor.

15 The user may then inhale through the fluid inlet 16 in order to move the plunger back from the end position to the start position, or alternatively push the plunger back manually.

20 In use, the plunger 6, movement switches 10, 12, and the oxygen sensor 8 comprise the means to measure the reference metabolic rate of a user from at least one breath.

25 In use, a user at rest will exhale into the apparatus 2, in order for the apparatus 2 to measure the reference metabolic rate. The reference metabolic rate may comprise readings from a single exhaled breath, or comprise an average from a plurality of exhaled breaths.

30

The apparatus 2 is of the size and configuration such that it can be held and carried in the hand by an individual

and connected to the electrical calculation means when desired.

Once a reference metabolic rate is established, a user may
5 subsequently breath into the apparatus 2, to measure the
metabolic rate from subsequent breaths. The electrical
calculation means 14 detect the metabolic rate of the user
from subsequent breaths, and compare it to the reference
metabolic rate.

10

If a deviation is detected from the reference metabolic
rate, then the device will indicate a deviation, through
use of an audio signal from a speaker (not shown), and the
electronic calculation means are then arranged to be
15 deactivated to prevent recordal of subsequent breaths.

The electronic calculation means 16 therefore comprises
the means to prevent measurement of subsequent breaths.

20 A user may then override the measurement prevention means
by pressing the button 50, which sends a signal to the
electronic calculation means 14 to reactivate, and measure
subsequent breaths by the user. In this way, breaths
which a user knows will be outside of the reference
25 metabolic rate, or believes would be outside of the
reference metabolic rate, can then be measured, in order
for the apparatus 2 to measure the raised or lowered
metabolic rate.

30 This is particularly useful for users who wish to measure
metabolic rate after a certain defined period of activity
or exercise.

For example, a user may breath into the apparatus 2 and the electronic calculations means 14 may calculate a reference metabolic rate of 1.5 Kcal/minute. A user may then undertake exercise for 10 minutes, and breath into the device, at which point the electronic calculation means 14, as the means to detect a deviation from the reference metabolic rate, will detect a raised metabolic rate, and prevent recordal of subsequent breaths. The speaker will audibly indicate to the user that a metabolic rate outside of the reference range has been detected, and the electronic calculation means 14 as the measurement prevention means, will deactivate to prevent recordal of subsequent breaths. The user may then press the button 50, to reactivate the electronic calculation means 14, and breath into the device to measure subsequent breaths after exercise. The electronic calculation means 14 can then calculate the raised metabolic rate utilising the plunger 6, movement sensors and oxygen sensor 6, and indicate the value of the raised metabolic rate to the user.

We refer now to Figure 3 which illustrates the second preferred embodiment of the breath monitoring apparatus of the invention. The breath monitoring apparatus 2 comprises a housing 100 in which is housed a means to measure the volume and gas content of an exhaled breath of a user (not shown). The means to measure the gas content of the exhaled breath comprises a City Technology 40X-1 City Cell Oxygen Meter (supplied by City Technology Ltd, Portsmouth, UK) and the means to measure the volume of the exhaled breath comprises a Honeywell AWM 5104 VN Mask Flow Meter (Honeywell, USA). The housing 100 also includes electronic calculation means (not shown) which comprise the means to calculate the reference metabolic rate of one

or more breaths in conjunction with the means to measure the gas content and volume of an exhaled breath of a user. The means to calculate the reference metabolic rate also comprise the means to measure metabolic rate from
5 subsequent breaths of a user.

Extending from one end of the housing 100 is a fluid inlet 102. A detachable mouthpiece 104 is connected to the fluid inlet 102. The mouthpiece 104 includes a T-valve
10 108, which allows exhaled breath to enter the fluid inlet 102 and into apparatus 2, but allows air from outside the apparatus 2 to be inhaled through the T-valve when a user inhales. The mouthpiece 104 includes the Mask Flow Meter, for measuring the volume of breath of the user. The
15 distal end of the T-valve includes a flexible mask 106, arranged to be connected over the mouth of a user.

The apparatus 2 includes a display screen 110, which acts as a means to indicate a deviation from the reference
20 metabolic rate in a breath. The display screen 110 displays text to a user.

The device includes means for preventing measurement of subsequent breaths upon detection of a deviation from the
25 reference metabolic rate, in the form of the electronic calculation means (not shown).

The apparatus 2 also includes means for user to override measurement prevention means to enable measurement of
30 metabolic rate from breaths which deviate from the reference rate, in the form of an actuator button 112.

Use of the device shown in Figure 3 is similar to that shown in Figures 1 and 2.

5 In use, a user will exhale into the apparatus 2 and the reference metabolic rate will be calculated by the electronic calculation means, from data supplied by the flow meter and oxygen sensor. The reference metabolic rate may be measured from a single exhalation or an average of a plurality of exhalations. The reference
10 metabolic rate may allow for deviation within a defined range, which may be set by a user or machine set.

Once the reference metabolic rate is determined, a user may then subsequently breathe into the apparatus 2, and
15 the electronic calculations means will measure the metabolic rate of subsequent breaths. If a deviation from the reference rate is detected, then this will be indicated on the display screen 110, and the electronic activation means will deactivate to prevent subsequent
20 breaths from being measured.

The user may override the measurement prevention means by pressing the activator button 112, which sends a signal to the electronic calculation means to reactivate and measure
25 the metabolic rate of subsequent breaths.

The reader's attention is directed to all papers and documents which are filed concurrently with or previous to this specification in connection with this application and
30 which are open to public inspection with this specification, and the contents of all such papers and documents are incorporated herein by reference.

All of the features disclosed in this specification (including any accompanying claims, abstract and drawings), and/or all of the steps of any method or process so disclosed, may be combined in any combination, except combinations where at least some of such features and/or steps are mutually exclusive.

Each feature disclosed in this specification (including any accompanying claims, abstract and drawings), may be replaced by alternative features serving the same, equivalent or similar purpose, unless expressly stated otherwise. Thus, unless expressly stated otherwise, each feature disclosed is one example only of a generic series of equivalent or similar features.

15

The invention is not restricted to the details of the foregoing embodiment(s). The invention extend to any novel one, or any novel combination, of the features disclosed in this specification (including any accompanying claims, abstract and drawings), or to any novel one, or any novel combination, of the steps of any method or process so disclosed.

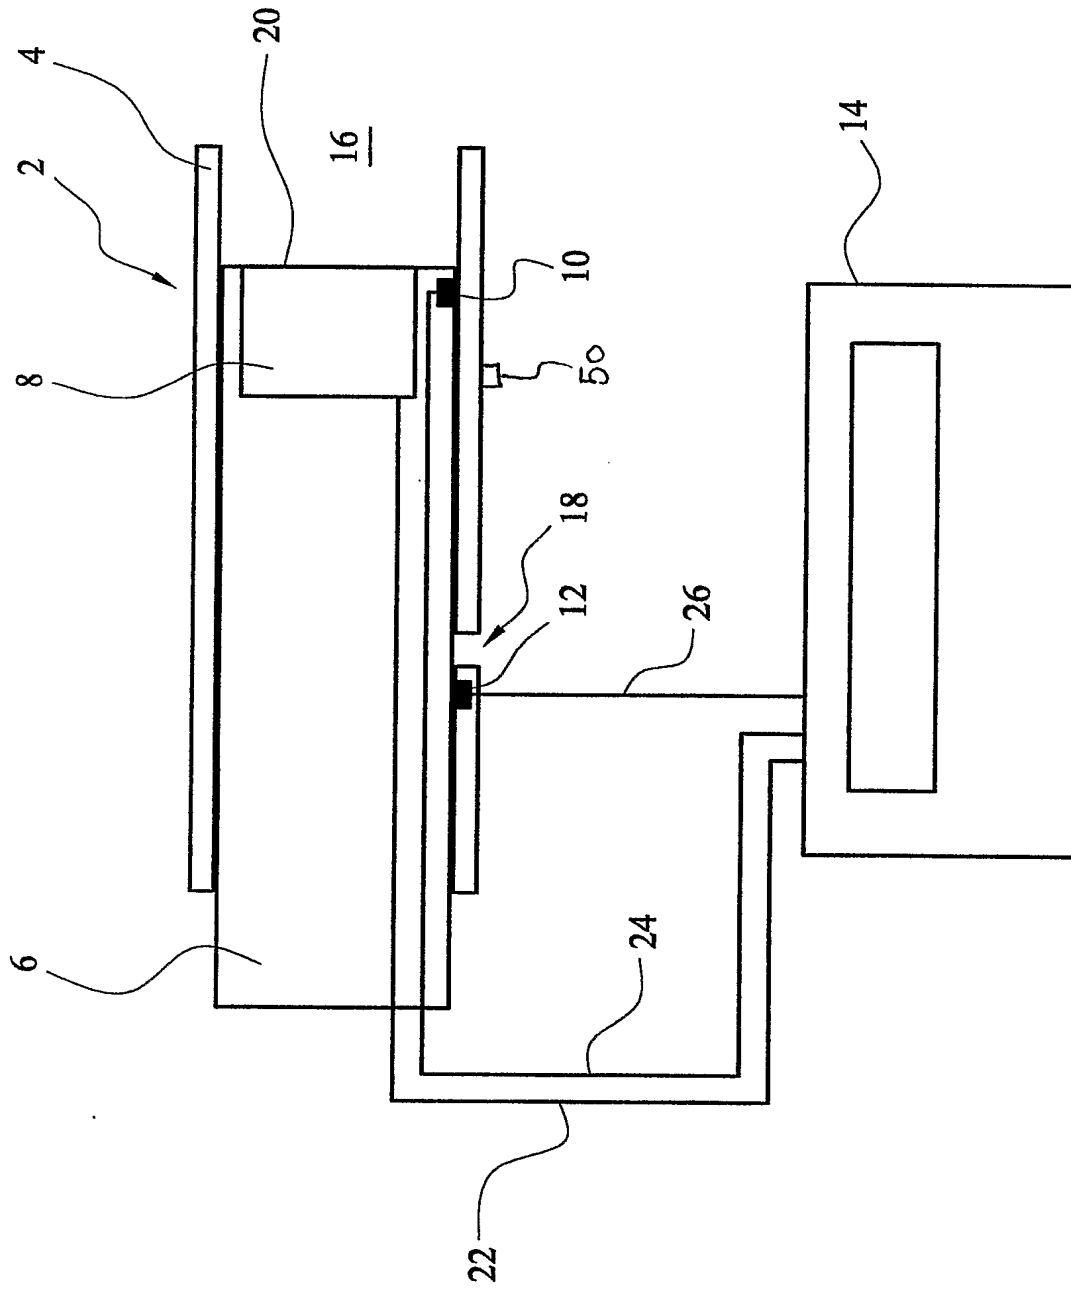


FIG. 1



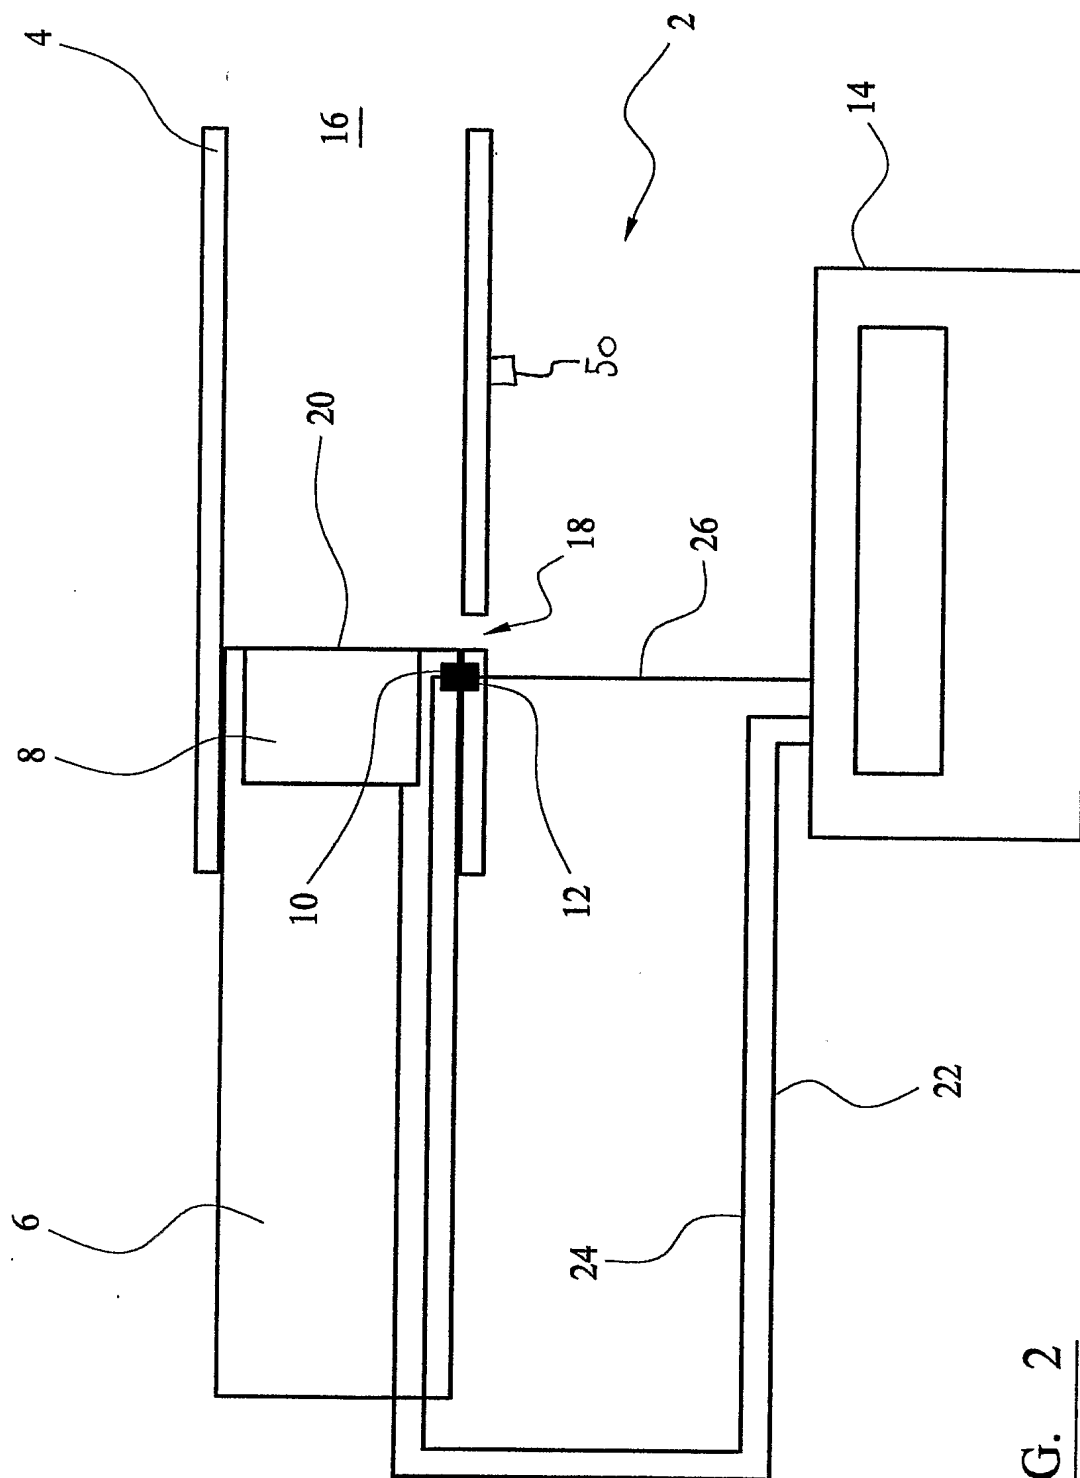


FIG. 2



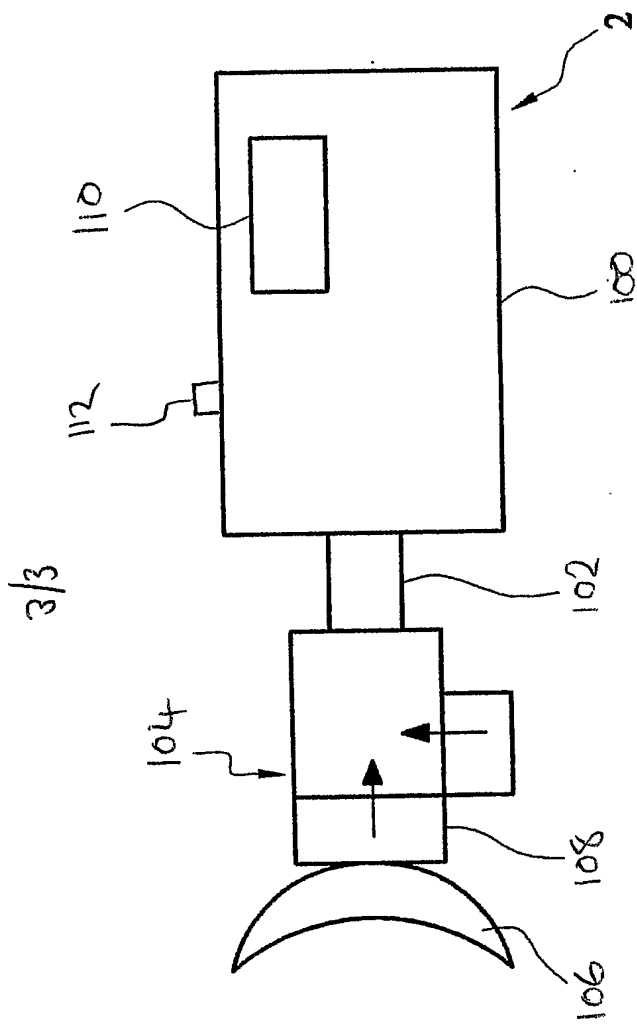


FIG. 3

